

AccuDiag™
Deoxynivalenol
ELISA Kit

REF 5147-8




Test	Deoxynivalenol ELISA
Recovery (spiked samples)	90-110%
Total Time	~ 60 min.
Shelf Life	12 Months from the manufacturing date
Specificity	N/A
Sensitivity	0.5 ng/mL

INTENDED USE

The Diagnostic Automation, Inc. Deoxynivalenol ELISA represents a highly sensitive detection system and is particularly capable of the quantification of deoxynivalenol contaminations in cereals, beer and soy.

General Information

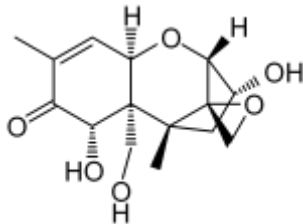

Deoxynivalenol (DON, Vomitoxin) in addition to zearalenone, the fumonisines and other trichothecenes belongs to the fusarium toxins. These toxins are already produced on the field in consequence of a contact of the cereals by fusarium species. Acute toxic dosages result in sickness and emesis. Deoxynivalenol is a gastrointestinal irritant and an inhibitor in protein synthesis. Farm animals react with a delay of growth and a depressed immune system resulting in a higher sensitivity for infections.

Since July 1st, 2006 the following maximum amounts of deoxynivalenol are valid throughout the EU:

Raw cereals	1250-1750 ppb
Flour	750 ppb
Bakery products	500 ppb
Baking ingredients (dry)	750 ppb
Baby food	200 ppb

Since June 2010 the FDA recommends maximum amounts of 1000 ppb for cereal products and 10000 ppb for raw cereals. Thus an observation of food and feed with respect to the concentration of deoxynivalenol is obligatory.

The Diagnostic Automation, Inc. Deoxynivalenol quantitative test is based on the principle of the enzyme-linked immunosorbent assay. An antibody binding protein is coated on the surface of a microtiter plate. Deoxynivalenol containing samples or standards and an antibody directed against deoxynivalenol are given into the wells of the microtiter plate. The deoxynivalenol contained in samples or standards will bind to the antibody which reacts with the binding protein coated onto the microtiter plate. After 30 minutes incubation at room temperature a deoxynivalenol-peroxidase conjugate is added into the wells without a preceding washing step to saturate free antibody binding sites. After additional 15 minutes incubation at room temperature the wells are washed with diluted washing solution to remove unbound material. A substrate solution is added and incubated for 15 minutes, resulting in the development of a blue colour. The colour development is inhibited by the addition of a stop solution, and the colour turns yellow. The yellow colour is measured photometrically at 450 nm. The concentration of deoxynivalenol is indirectly proportional to the colour intensity of the test sample.

MATERIALS AND COMPONENTS

Materials provided with the test kits

The kit contains reagents for 96 determinations. They have to be stored at 2-8°C.

Expiry data are found on the labels of the bottles and the outer package.

1. **Microtiter plate** consisting of 12 strips with 8 breakable wells each, coated with anti-mouse antibody.
2. **Deoxynivalenol Standards (0, 2, 8, 20, 40, 80 ng/mL)**: 6 vials with 1 mL each, dyed red, ready-to-use.
3. **Anti-Deoxynivalenol Antibody (mouse)**: 6 mL, dyed red, ready-to-use.
4. **Conjugate (Deoxynivalenol-Peroxidase)**: 6 mL, dyed red, ready-to-use.
5. **Substrate Solution (TMB)**: 15 mL, prestained red, ready-to-use.
6. **Stop Solution (0.5 M H₂SO₄)**: 15 mL; ready-to-use.
7. **Sample Diluent (PBS)**: 2 x 60 mL; dyed red, ready-to-use.
8. **Washing Solution (PBS + Tween 20)**: 60 mL as 10x concentrate. Dilute 1+9 with distilled water. If during the cold storage crystals precipitate, the concentrate should be warmed up at 37°C for 15 minutes.
9. Two plastic foils to cover the strips during the incubation.
10. Plastic bag to store unused microtiter strips.
11. Instruction Manual.

Materials required but not provided

1. 50, 100 and 1000 µL-micropipettes
2. ELISA reader (450 nm)
3. Centrifuge
4. Ultra-Turrax, mixer, vortex

Reagents

1. Double distilled water
2. Potassiumhexacyanoferrate(II)-3-hydrate (150 g/L; Carrez I)
3. Zinculfate-7-hydrate (300 g/L; Carrez II)

Sample Preparation

Cereals

1. Suspend 4 g of previously ground sample in 20 mL of double distilled water.
2. Mix suspension for 5 minutes.
3. Centrifuge extract at 3000 g for 10 minutes.
4. Dilute 200 µL of supernatant with 800 µL of sample diluent and test the sample in the ELISA.
5. Sample dilution factor: F=25.


Beer / Gyle

1. Carbonized beer samples should be previously degassed by moderate heating.
2. Cloudy beers (such as beer brewed from wheat) / gyle should previously be sterile-filtered.
3. Dilute 100 µL beer / gyle with 900 µL sample diluent.
4. Sample dilution factor: F=10.

Soy

1. Suspend 4 g of previously ground sample in 20 mL of double distilled water.
2. Mix suspension for 5 minutes.
3. Centrifuge extract at 3000 g for 10 minutes.
4. Add 100 µL Carrez I to 1 mL supernatant, mix well and add 100 µL Carrez II afterwards.
5. Mix sample and centrifuge at 3000 g for 10 minutes.
6. Dilute 250 µL of supernatant with 800 µL of sample diluent and test the sample in the ELISA.
7. Sample dilution factor: F=25.

Deoxynivalenol (ng/mL)	(% binding of 0 ng/mL)
0	100
2	84
8	58
20	34
40	22
80	15

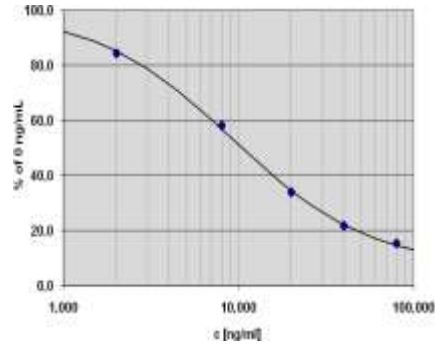

ASSAY PROCEDURE

1. Prepare samples as described above.
2. Pipette 100 µL standards or prepared samples in duplicate into the appropriate wells of the microtiter plate. Immediately add 50 µL anti-deoxynivalenol antibody into each well.
3. Cover the microtiter plate with a plastic foil and incubate for 30 minutes at room temperature.
4. Without preceding washing add 50 µL deoxynivalenol-peroxidase conjugate into each well.
5. Cover the microtiter plate with a plastic foil and incubate additional 15 minutes at room temperature.
6. Wash the plate three times as follows: Discard the contents of the wells (dump or aspirate). Pipette 300 µL of diluted washing solution into each well. After the third repetition empty the wells again and remove residual liquid by striking the plate against a paper towel. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbencies.
7. Pipette 100 µL of substrate solution into each well.
8. Allow the reaction to develop in the dark (e.g. cupboard or drawer; the chromogen is light-sensitive) for 15 minutes at room temperature.
9. Stop enzyme reaction by adding 100 µL of stop solution (0.5 M H₂SO₄) into each well. The blue colour will turn yellow upon addition.
10. After thorough mixing, measure absorbance at 450 nm (reference wavelength 620 nm), using an ELISA reader. The colour is stable for 30 minutes.

RESULTS

1. Calculate the average optical density (OD 450 nm) for each set of reference standards or samples.
2. Construct a standard curve by plotting the mean optical density obtained for each reference standard against its concentration in ng/mL on semi-log graph paper with the optical density on the vertical (y) axis and the concentration on the horizontal (x) axis.
3. Using the mean optical density value for each sample, determine the corresponding concentration of deoxynivalenol in ng/mL from the standard curve. Depending on experience and/or the availability of computer capability, other methods of data reduction may be employed.
4. The diluted samples must be further converted by the appropriate **sample dilution factor**. The factors are listed for each sample matrix in the *sample preparation* section.

Typical Standard Values

The following table contains an example for a typical standard curve. The binding is calculated as percent of the absorption of the 0 ng/mL standard. These values are only an example and should not be used instead of the standard curve which has to be measured in every new test.

PERFORMANCE CHARACTERISTICS

Sensitivity

The limit of detection (LOD) of the **Diagnostic Automation, Inc. Deoxynivalenol test** is 0.5 ng/mL.

The limit of quantification (LOQ) of the **Diagnostic Automation, Inc. Deoxynivalenol test** is 2 ng/mL.

Due to the variety of sample matrices and their influence on the blank, results less than the LOQ should be treated as negative.

Recovery

Wheat flour	106%
Maize flour	97%
Beer	99%
Soy	90%

Intra-assay Precision

The intra-assay variation of the deoxynivalenol test was determined to 5%.

Cross-reactivity relative to deoxynivalenol (=100%)

15--acetyl-Deoxynivalenol	0.4%
3-acetyl-Deoxynivalenol	800 %

PRECAUTION

Full compliance of the following good laboratory practices (GLP) will determine the reliability of the results:

1. Prior to beginning the assay procedure, bring all reagents to room temperature (20-25°C).
2. All reagents should be mixed by gentle inversion or swirling prior to use. Do not induce foaming.



3. Once the assay has been started, all subsequent steps should be completed without interruption and within the recommended time limits.
4. Replace caps in all the reagents immediately after use. Do not interchange vial stoppers.
5. Use a separate disposable tip for each specimen to prevent cross-contamination.
6. All specimens and standards should be run at the same time, so that all conditions of testing are the same.
7. Do not mix components from different batches.
8. Do not use reagents after expiration date.
9. Check both precision and accuracy of the laboratory equipment used during the procedure (micropipette , ELISA reader etc.)

Health and safety instructions

1. Do not smoke or eat or drink or pipette by mouth in the laboratory.
2. Wear disposable gloves whenever handling patient specimens.
3. Avoid contact of substrate and stop solution with skin and mucosa (possible irritation, burn or toxicity hazard). In case of contact, rinse the affected zone with plenty of water.
4. Handling and disposal of chemical products must be done according to good laboratory practices (GLP).

REFERENCES

1. Barros G, et al. (2008) – Deoxynivalenol and nivalenol analysis in soybean and soy flour. *W of Myc J*, 1(3):263-266
2. Chidozie J, et al.(2009) – Supression of insulin-like growth factor acid-labile subunit expression – a novel mechanism for don-induced growth retardation. *Toxic Sci*, 113(2):412-421
3. Sobrova P, et al. (2010) – Deoxynivalenol and its toxicity. *Interd Tox*, 3(3):94-99
4. Papadopoulou-Bouraoui, et al. (2004) - Screening survey of deoxynivalenol in beer from the European market by an enzyme-linked immunosorbent assay. *Food Addit Contam*, 21(6):607-17
5. Wolf-Hall CE, et al. (1999) – Stability of deoxynivalenol in heat-treated foods. *J Food Prot*, 62(8):962-964
6. Jajić I, et al. (2008) – Occurence of deoxynivalenol in maize and wheat in Serbia. *Int J Mol Sci*, 9:2114-2126
7. Zachariasova M, et al. (2008) – Deoxynivalenol and its conjugates in beer. *Anal Chim Acta*, 625(1):77-86
8. Suproniene S, et al. (2010) – Distribution of trichothecene and zearalenone producing fusarium species in grain of different cereal species and cultivars grown under organic farming conditions in Lithuania. *Ann Agric Environ Med*, 17:79-86
9. Sifuentes dos Santos, et al. (2011) – Immunoassay based on monoclonal antibodies versus LC-MS: deoxynivalenon in wheat and flour in Southern Brazil. *Food Addit Contam Part A Chem Anal Control Expo Risk Assess*, 1:1-8
10. Yoshizawa T, et al. (2004) – A practical method for measuring deoxynivalenol, nivalenol and T-2 + HT-2 Toxin in foods by an enzyme linked immunosorbent assay using monoclonal antibodies. *Biosci Biotech Biochem*, 68(10):2076-2085

ISO 13485 ISO 9001 	
 Diagnostic Automation/Cortez Diagnostics, Inc. 21250 Califa Street, Suite 102 and 116, Woodland Hills, California 91367 USA	
Date Adopted	2015-10-19
REF 5147-8	AccuDiag™ - Deoxynivalenol ELISA
Revision Date:2014-02-21	